

COMPOUND DATA SHEET

FM140/0 Grey

General description

FM140/0 is a chlorobutyl compound with silicate filler. Unconventionally cured.

Identification as per Ph.Eur. 3.2.9., method A

A typical ATR-FTIR spectrum of a clean, cut surface of FM140/0 is enclosed on page 3.

Physical properties

Hardness <i>ISO 7619-1 (1sec Indentation)</i>	46 ± 5 °Shore A
Density <i>ISO 2781</i>	1.323 ± 0.025 g/cm ³
Ash content <i>Internal method. Calc.4h @700°C</i>	45.5 ± 2.0 %
Compression set <i>ISO 815, (typical value)</i>	32 %
Modulus 100 <i>Internal method. 100mm/min, (typical value)</i>	1.3 N/mm ²
Modulus 300 <i>Internal method. 100mm/min, (typical value)</i>	2.0 N/mm ²
Elongation @ Break <i>Internal method. 200mm/min, ISO 37 Dumb-bell 2, (typical value)</i>	670 %
Tensile Strength @ Break <i>Internal method. 200mm/min, ISO 37 Dumb-bell 2, (typical value)</i>	6.6 N/mm ²
Water Vapor Transmission Rate <i>Mocon, 38°C, 100%RH, 1.27 mm thickness, (typical value)</i>	0.06 g/m ² .24h
Oxygen Transmission Rate <i>Mocon, 38°C, 90%RH, 100% O₂, 1.27 mm thickness, (typical value)</i>	71 cc/m ² .24h

Compound ingredient declarations

Latex	FM140/0 is not made with natural rubber latex.
Nitrosamines	FM140/0 is not made with chemicals that are associated with nitrosamine formation as per the ASTM F1313-90 list.
Phthalates	FM140/0 is not made using Di(2-EthylHexyl) Phthalate (DEHP) or other phthalates.
BSE/TSE	For the raw materials of FM140/0, certification confirming that such products are either of vegetable origin or are manufactured in severe process conditions for inactivation of prions as described in the EMA/410/01-rev.3 and in the European Pharmacopoeia 5.2.8. "Minimizing the risk of transmitting Animal Spongiform Encephalopathy Agents" is available.
MBT	FM140/0 is not made with 2-mercapto-benzothiazole (MCBT, also named MBT), or any of its derivatives.
Heavy Metals	FM140/0 fulfills the EC Guideline 94/62/EC for heavy metals in packaging materials and the CONEG regulation on reduction of toxics in Packaging Law: "packaging components shall not contain more than 100 ppm of Pb, Cd, Hg, and Cr(VI)".

Chemical properties

Ph.Eur.3.2.9. : FM140/0 meets the chemical requirements for **ISO 8871-1** Type I closures specified in Ph.Eur. 3.2.9, ISO 8871-1 and USP <381>. **USP <381>** Typical results are given in the table on page 2. Typical UV spectra are enclosed on page 3.




Ph.Jap.7.03. : FM140/0 meets the chemical requirements specified in Ph.Jap. 7.03. Typical results are given in the table on page 2.

Note : Chemical testing is performed on non-post-treated standard test plates or products, prepared using representative process conditions.

Biocompatibility

USP <87><88>: FM140/0 is non-cytotoxic and meets the requirements of the Elution Test as described in USP <87>,"Biological Reactivity Tests, in vitro" and the ISO 10993-5 "in vitro cytotoxicity". A typical test certificate is enclosed on page 4. **ISO 10993-5** cytotoxicity testing is considered equivalent with Pharm. Jap. 7.03 cytotoxicity testing.

Note : "FMxxx" refers to the type of compound, the extension "x" refers to the color of the said compound. Differently colored compounds might be used for testing throughout this document. It is generally accepted that the color is irrelevant for the properties discussed, except Ash content and Density which are different per color.

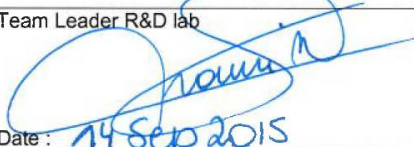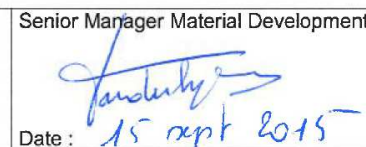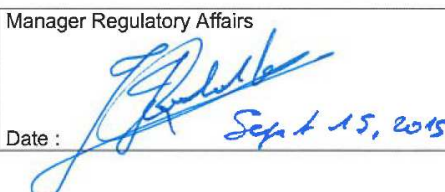Team Leader R&D lab  Date: 14 Sep 2015	Senior Manager Material Development  Date: 15 sept 2015	Manager Regulatory Affairs  Date: Sept 15, 2015
---	--	--

COMPOUND DATA SHEET

FM140/0 Grey

Typical results of chemical properties as per the Ph.Eur.3.2.9., ISO 8871-1 and the USP <381> for FM140/0:

Characteristic		Limits		FM140/0
Appearance of solution	Turbidity	Type I: ≤ 6 NTU (*) Type II: ≤ 18 NTU (*)		0
	Color	Solution S is not more intensely colored than reference		Pass
Acidity or alkalinity (NA : Not applicable)	≤ 0.8 ml 0.01M HCl	EP		NA
		USP**		NA
	≤ 0.3 ml 0.01M NaOH	EP		0.1
		USP**		0.0
UV Absorbance (max 220-360 nm)	Type I: ≤ 0.2 Type II: ≤ 4.0		0.0	
Reducing substances	Type I: ≤ 3.0 ml 0.01M Na ₂ S ₂ O ₃ Type II: ≤ 7.0 ml 0.01M Na ₂ S ₂ O ₃		0.2	
Extractable heavy metals	≤ 2 ppm Pb ²⁺	EP		Pass
		USP***		Pass
Extractable zinc	≤ 5.0 ppm Zn ²⁺		0.3	
Ammonium	≤ 2 ppm NH ₄ ⁺		Pass	
Residue on evaporation (only for EP)	Type I: ≤ 2.0 mg Type II: ≤ 4.0 mg		0.1	
Volatile sulphides	Any black stain on the paper is not more intense than that produced by a control solution		Pass	

(*) By definition corresponding with reference suspensions II and III (for Ph.Eur.) or B and C (for USP) respectively

(**) Corrected with blank

(***) Measured as per USP <231>; USP <231> will become obsolete by Dec 1, 2015

Typical results of chemical properties as per the Ph.Jap.7.03 for FM140/0:


Characteristic		Limits	FM140/0
Appearance	%T at 430nm	$\geq 99.0\%$	99.6
	%T at 650nm	$\geq 99.0\%$	99.8
pH (difference with blank)	$-1.0 \geq \leq 1.0$		-0.1
Zinc	≤ 1 ppm Zn ²⁺		0.4
Reducing substances	≤ 2.0 ml 0.002 M KMNO ₄		0.7
Residue on evaporation	≤ 2.0 mg		0.2
UV absorbance (Max. Abs. 220-350nm)	≤ 0.20		0.02
Cadmium*	≤ 5 ppm		0.01
Lead*	≤ 5 ppm		1.10

(*) measured directly on the rubber



COMPOUND DATA SHEET

FM140/0 Grey

Typical ATR-FTIR spectrum of a clean, cut surface of FM140/0:

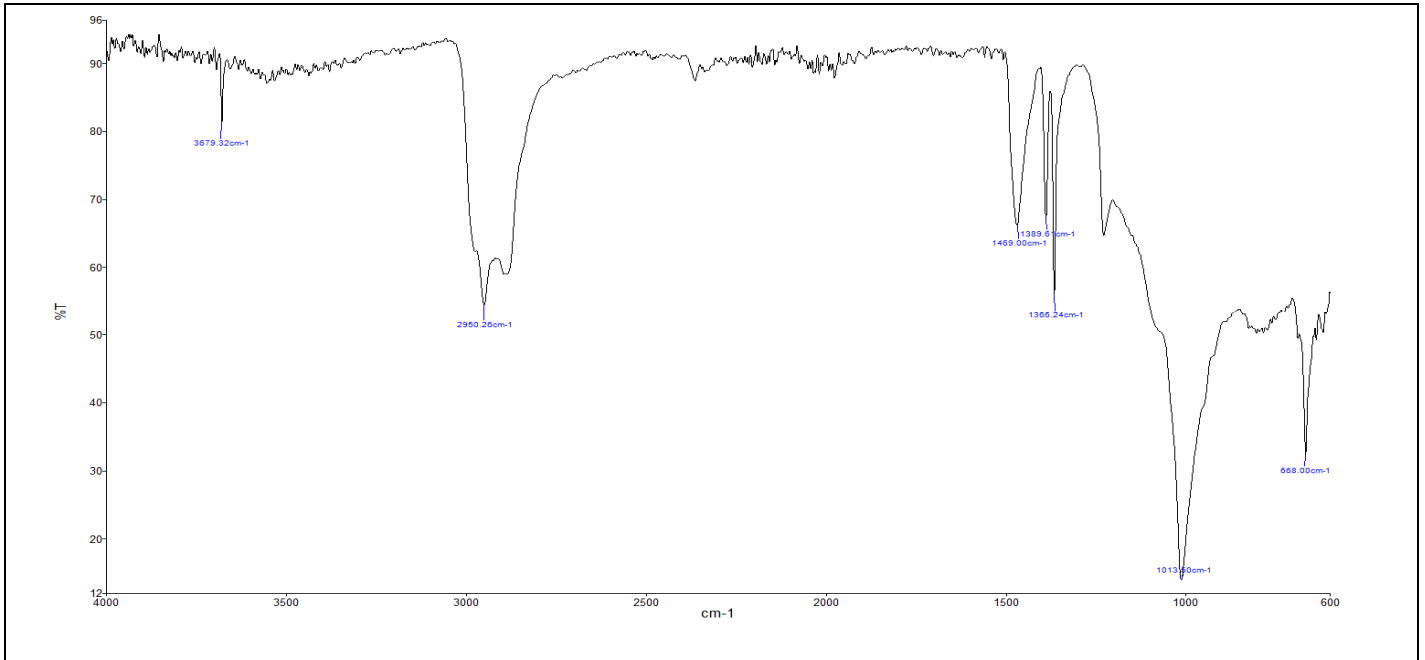

Typical UV spectrum of the Solution S extract of FM140/0, measured as per the Ph.Eur. 3.2.9., ISO8871-1 and USP <381> (left) and Ph.Jap.7.03 (right):

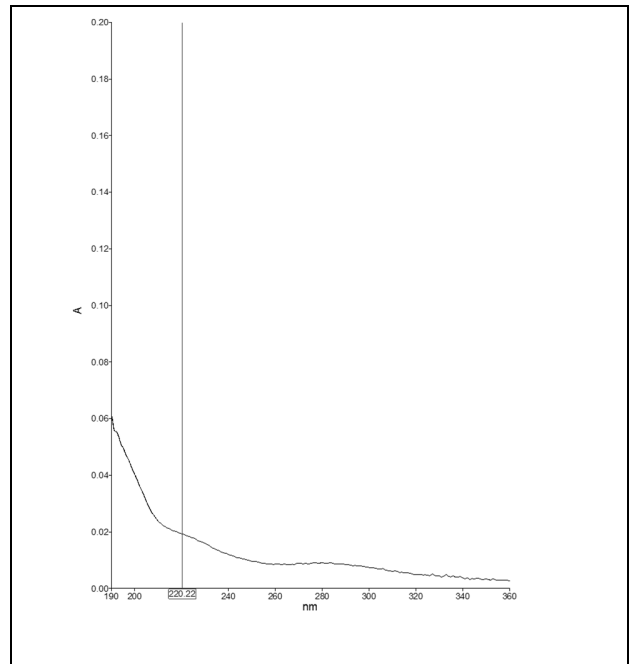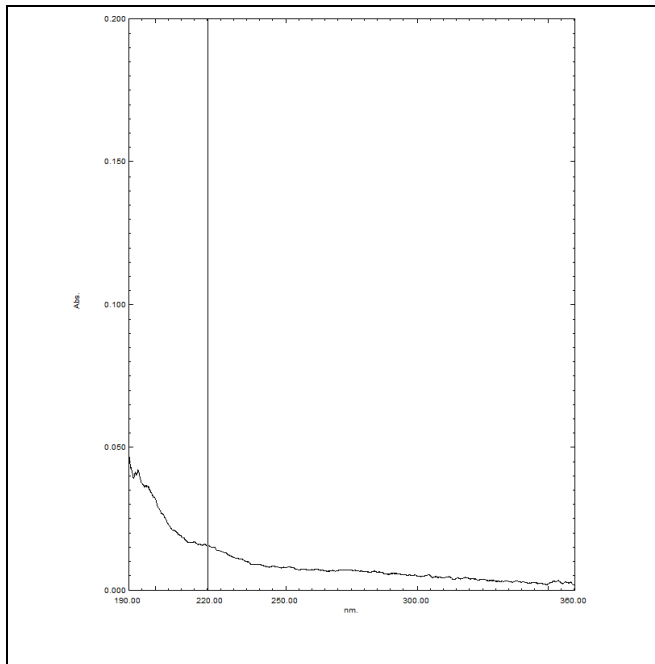



COMPOUND DATA SHEET

FM140/0 Grey

USP<87> Elution Test certificate for FM140/0:



TEST RESULT REPORT N°:10-B0277-N1

Project Number: TE 10118	Study Number: 10-B0277-N1
Sponsor: Helvoet Pharma Belgium NV	Report Date: 18/02/2010
Contact: Mrs. Nadia Nouri	
Address: Industrierterrein Kolmen 1519	Date Sample Arrival: 10/02/2010
3570 Alken, Belgium	Technical Initiation: 15/02/2010
PO.Number: PB1000518	Technical Completion: 18/02/2010

Study	Elution Test - ISO	Temp/Time	37°C/24 hours
Test Item	FM140/0 V9025 SAF1	Ratio	25cm ² /20mL
Lot	30194939	Vehicle	MEM-Complete

REFERENCE: According to "ISO 10993-5, 2009: Biological Evaluation of Medical Devices- Part 5: Tests for In Vitro Cytotoxicity," and "USP 32-NF 27, 2009: <87> Biological reactivity test, in vitro." Toxikon Reference: SOP 3.1.2.3, rev. 08

PROCEDURE: The biological reactivity of a mammalian monolayer, L929 mouse fibroblast cell culture, in response to the test item extract was determined. The samples and control articles were autoclaved prior to the preparation of the extracts. Extracts were prepared at 37±1°C for 24 hours in a humidified atmosphere containing 5±1% carbon dioxide (static). Positive (natural rubber) and negative (silicone) control articles were prepared to verify the proper functioning of the test system. The maintenance medium on the cell cultures is replaced by the extracts of the test item or control article in triplicate and the cultures are subsequently incubated for 48 hours, at 37±1°C, in a humidified atmosphere containing 5±1% carbon dioxide. Biological reactivity was rated on the following scale: Grade 0 (No reactivity); Grade 1 (Slight reactivity), Grade 2 (Mild reactivity), Grade 3 (Moderate reactivity) and Grade 4 (Severe reactivity). The test item is considered non-cytotoxic if none of the cultures exposed to the test item shows greater than mild reactivity (Grade 2).

OPINION AND INTERPRETATION: No reactivity (Grade 0) was exhibited by the cell cultures exposed to the test item at the 48 hours observation. Severe reactivity (Grade 4) was observed for the positive control article. The negative control article showed no signs of reactivity (Grade 0).

OPINION AND INTERPRETATION: Based on the evaluation criteria mentioned above, the test item is considered non-cytotoxic.

RECORD STORAGE: All raw data generated in this study will be archived at Toxikon Europe, according to SOP 4.2.8.

AUTHORIZED PERSONNEL

ir. Peter Cornelis
Study Director

Vanessa Ruymen
Quality Assurance

The test results on the enclosed report are only referring to the tested articles. Partly reproduction of this report can only be allowed after written permission of Toxikon. Toxikon guarantees that all results are acquired by testing according to officially accepted scientific methodology.

Toxikon Europe nv - Researchpark Haasrode 1724 - Romeinsestraat 12, B 3001 Leuven, Belgium - Tel. 32-16-40 04 84 - Fax 32-16-40 13 04
Fortis 230-0391575-06 - KBC 431-0597001-33 - BTW/TVA BE 0442.395.719 - H.R. Leuven 80.154 - www.toxikon.be